



# SITE INFORMATION AND EQUIPMENT LIST

---

## Injections Skill Examination (*ISE*®)

**August 2018 – July 2019**

---


The information listed in this Site Information and Equipment List is for informational purposes only. There may be additional equipment or supplies on-site during the exam that may not be reflected in this manual. Additionally, equipment and supplies may change without warning.

This information is not intended to prepare Candidates for the exam, but instead is intended to provide a general overview of equipment and supplies used during the exam. Candidates are reminded to thoroughly review the Evaluation Forms and Candidate Guide to adequately prepare for the Injections Skill Examination.

## Station Information - Lighting

### Main Overhead Light Switch Dimmer Switch & Slider

- Located behind computer workstation
- Location of this switch is the same in EVERY exam room
- Main Overhead Light Switch is located on the LEFT
- Dimmer switch is located on the RIGHT
- Slider to adjust dimmer brightness is on the RIGHT side of the dimmer switch

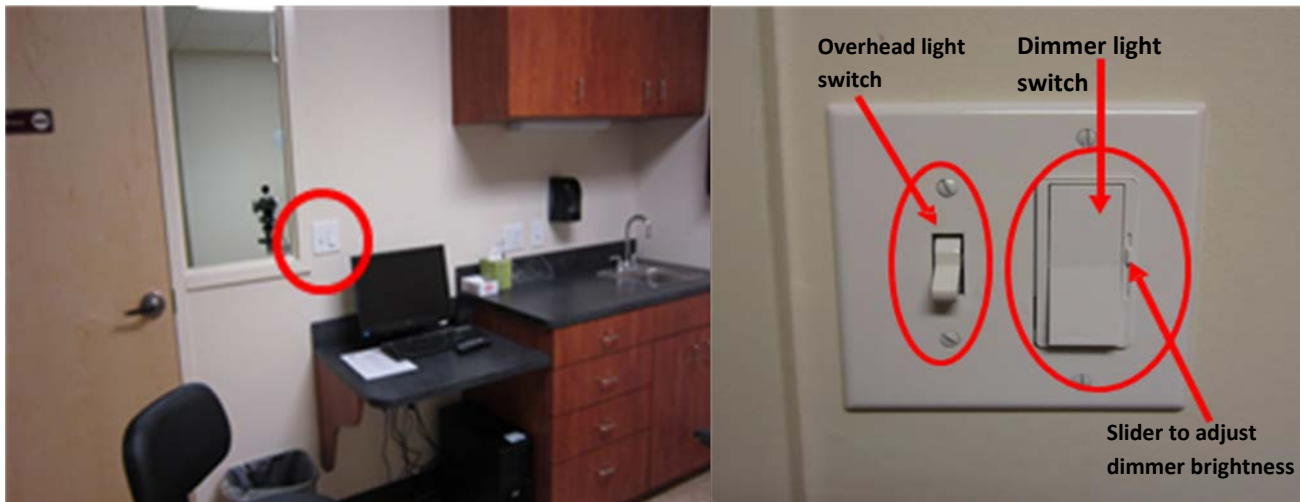

### Under Cabinet Light Switch


- Located above sink counter, by soap dispenser
- Location of this switch is the same in EVERY exam room.



# Station Information – Countdown Clock

Countdown clocks on the computers are **NOT THE OFFICIAL CLOCKS** that determine a candidate's time.

A countdown clock will be minimized on the menu bar at the bottom of the screen:

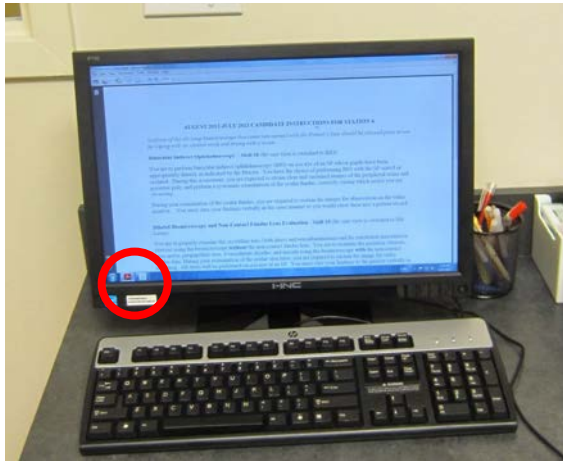


Candidates wishing to use the countdown clock will need to click on the menu bar to be able to start the countdown.

Once the announcement begins to play, that is when official testing time begins. Once the announcement plays ending the exam, time ends. Candidates wishing to use the countdown clock in the rooms must press the START button to begin the countdown clock. There will always be a delay between when the announcement plays and when a candidate presses START thus the time on the computer will always be less than 15 minutes. Using the countdown clock in the room is optional and only to provide Candidates assistance in determining the amount of time, digitally, remaining in the station. Again, these clocks are not the official time keepers of the exam.



“CLEAR” will reset the timer to 15 minutes. Candidates can minimize the timer by clicking on the minimize button located in the upper right corner:




The clock will continue to countdown minimized on the menu bar.



Here is a link to the timer that is available in the exam room: <http://www.online-stopwatch.com/countdown/>

# Station Information

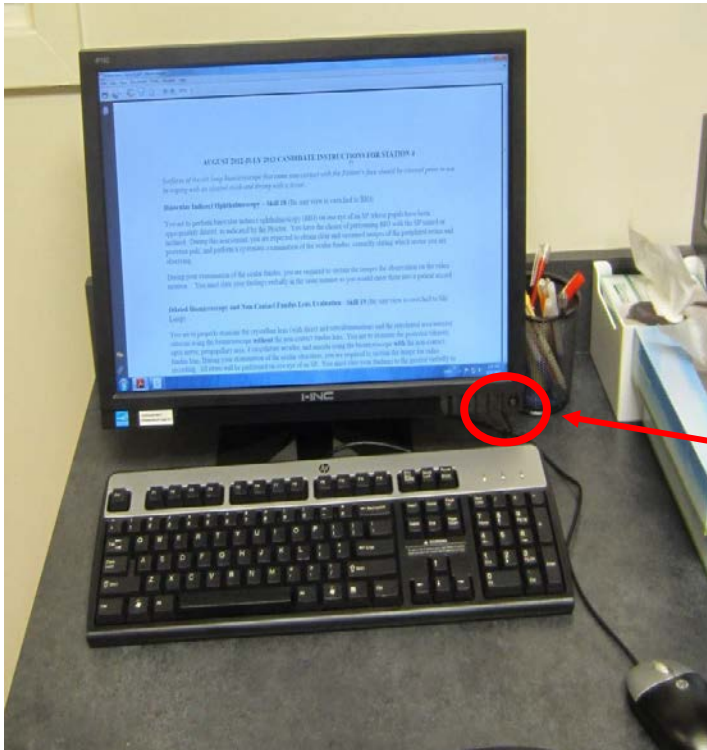

## Computer Workstations

Displays Station Instructions  
Not an item-by-item list, but a  
brief overview of Skills  
expected to be performed.

Turn the Monitor off/on by  
pressing the button on the  
bottom right corner

## Repeat Policies

Posted on the back of the  
exam room doors, next to the  
computer workstation

Pens & Pencils are  
provided in each  
Station for  
Candidate use

Band-Aids are  
available in all  
Stations in the event  
an injury occurs



# Station Equipment & Supplies

## Room View



## Station Room View Injections Area



# Injections Equipment & Supplies

Life/Form Advanced Venipuncture and Injection Arm



## Injections Supplies Overview

Injections supplies are organized in “buckets” on the table with plenty of needles, syringes, drape kits, etc.


Gloves/Tissues are found on the wall, to the right of the table.

Sharps containers are mounted directly above the injections table.



There will be 2 vials of each simulated medication available.



# Injections Equipment & Supplies

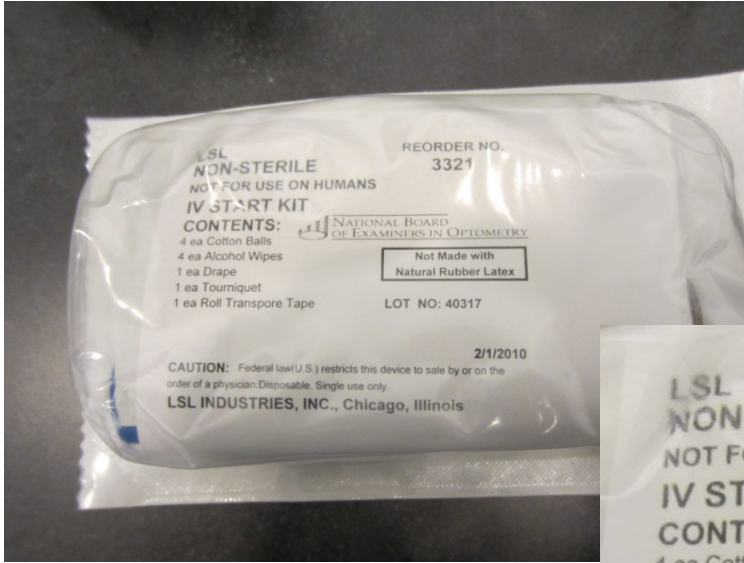

The Drape Kit will provide everything necessary to **simulate** an aseptic field for the injections exam.

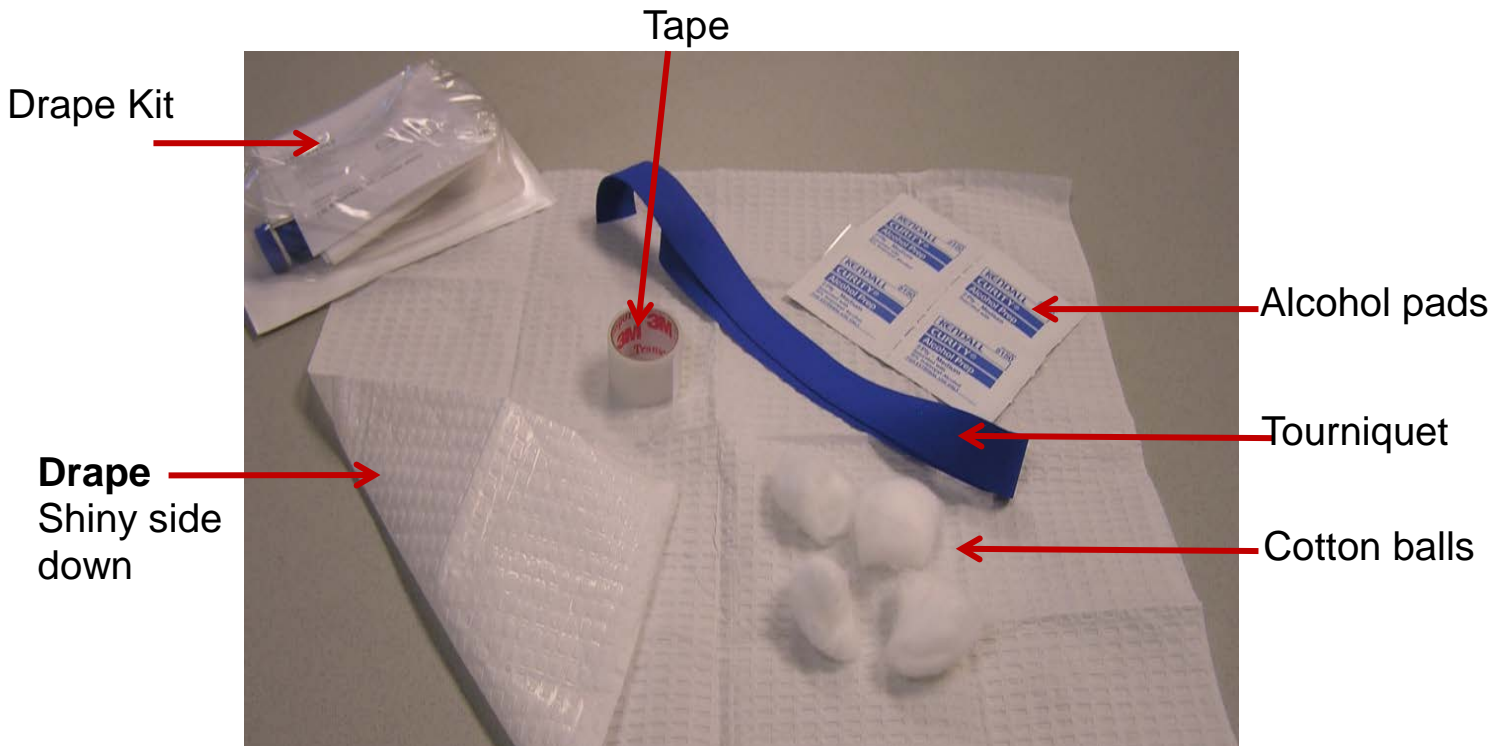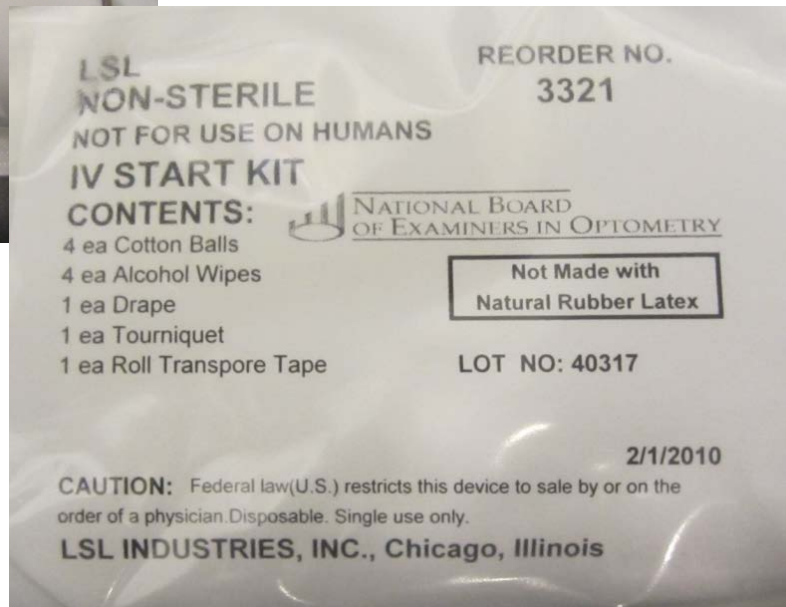

# Injections Equipment & Supplies

## Syringes

Brand may vary



1 cc Syringe  
for Epinephrine

5 cc Syringe  
for Fluorescein

## 25 Gauge Needles

Color/Brand may vary



## Butterfly / Winged Infusion Needle Sets 25 Gauge

Color/Brand may vary



Some Items may have plastic guards.  
The guards will need to be removed prior to use.  
Examples below.

